
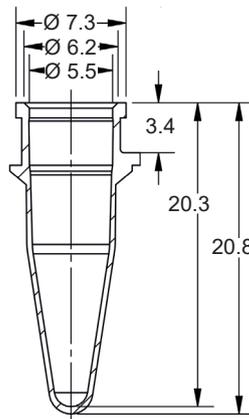
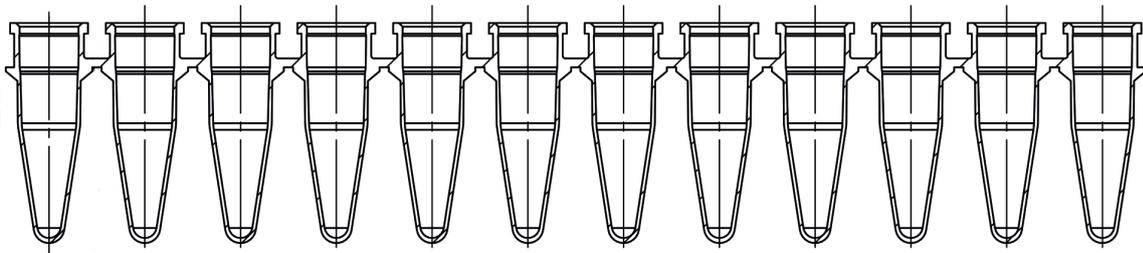


Strip of 8 PCR Tubes, 0.2 ml 781280

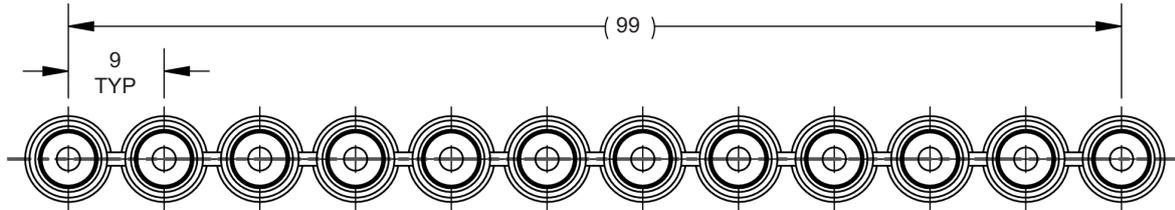

Dimensions in mm


Type	standard
Volume	0.2 ml / tube
Material	PP
Color	transparent
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.

Strip of 8 PCR Tubes, 0.2 ml, with cap 781315

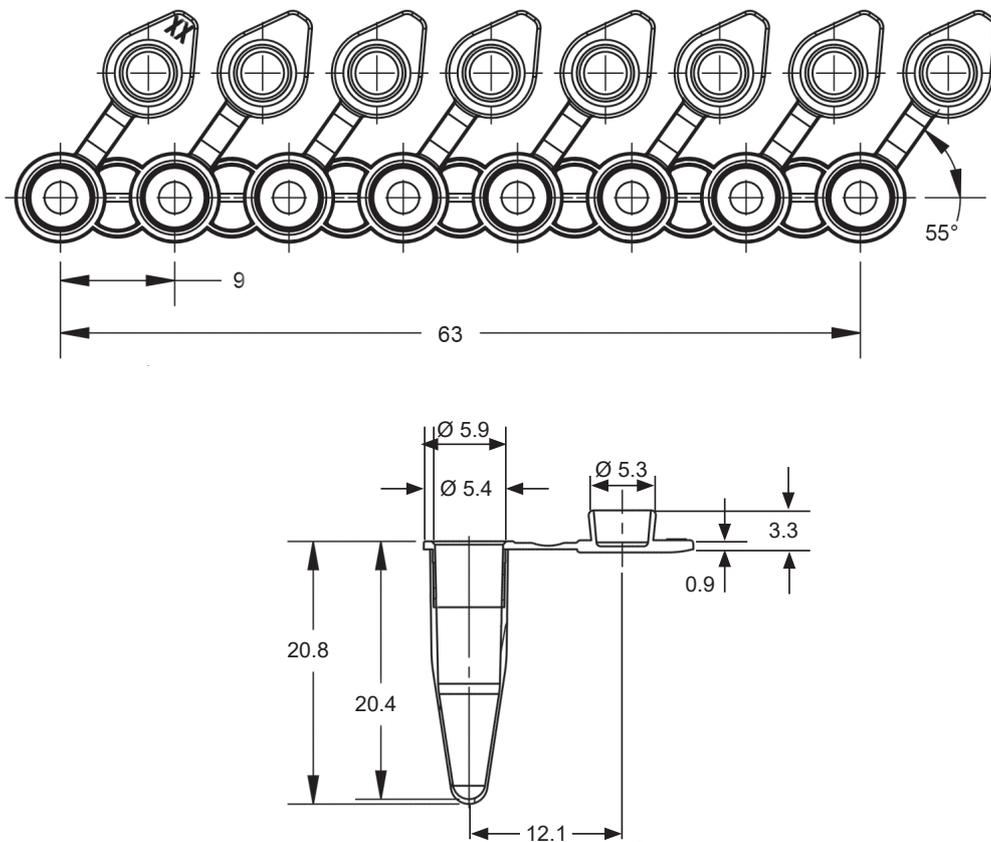

Dimensions in mm

Type	standard
Volume	0.2 ml / tube
Material	PP
Color	transparent
Cap	attached, flat individual cap
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.



02.51.12.70.01


Batailler-labo.fr



Contact@batailler-labo.fr

Strip of 8 PCR Tubes, 0.2 ml, with cap

781316

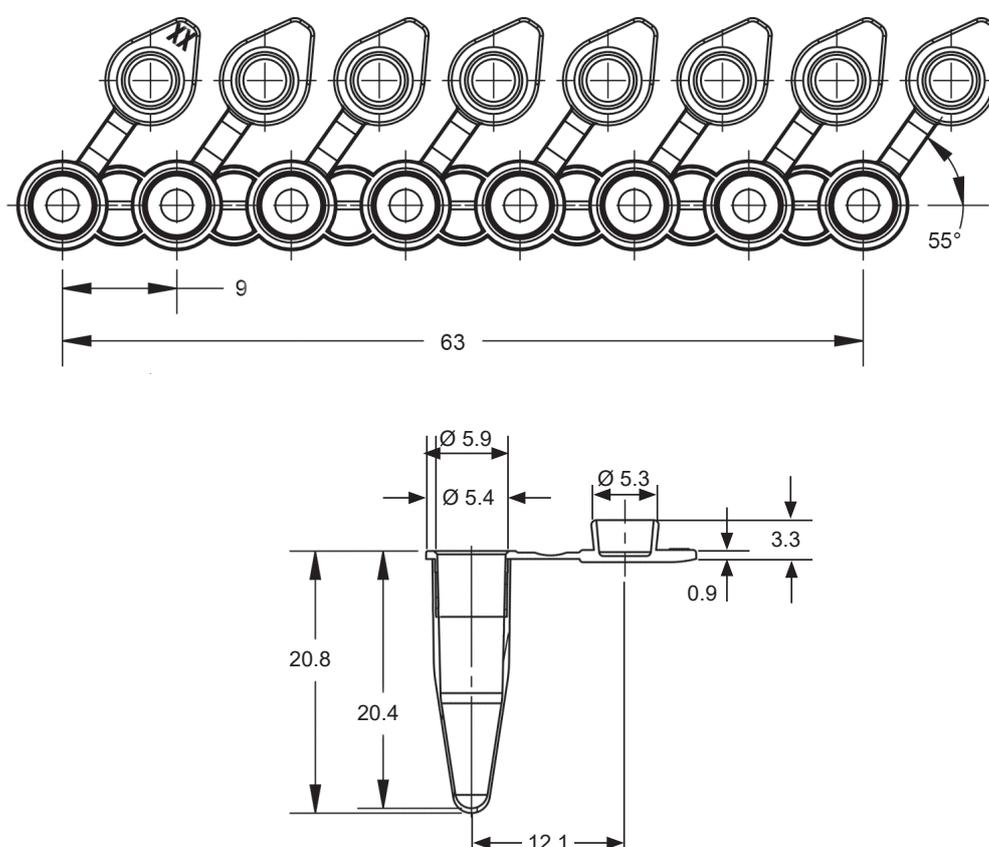

Dimensions in mm

Type	standard
Volume	0.2 ml / tube
Material	PP
Color	white
Cap	attached, flat individual cap
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.





02.51.12.70.01

Batailler-labo.fr



Contact@batailler-labo.fr

Strip of 8 PCR Tubes, 0.15 ml, with cap 781317

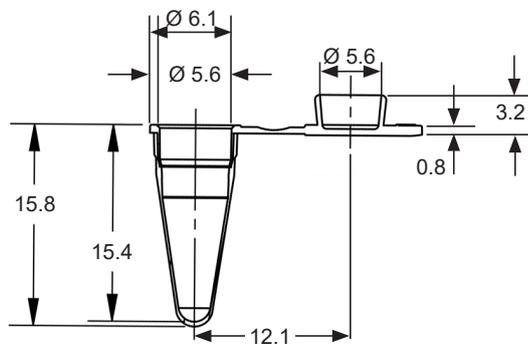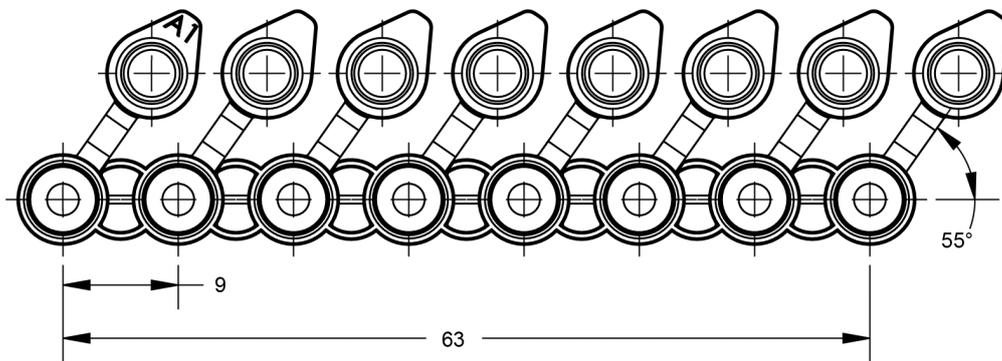

Dimensions in mm

Type	low profile
Volume	0.15 ml / tube
Material	PP
Color	white
Cap	attached, flat individual cap
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.





02.51.12.70.01

Batailler-labo.fr



Contact@batailler-labo.fr

Strip of 8 PCR Tubes, 0.15 ml, with cap 781318

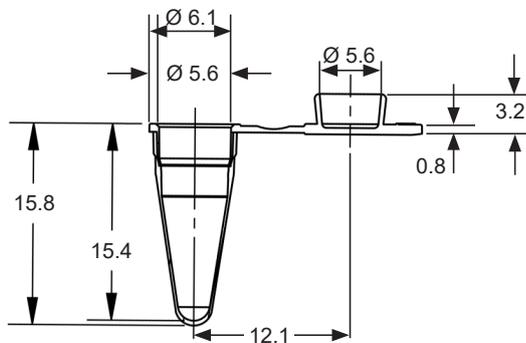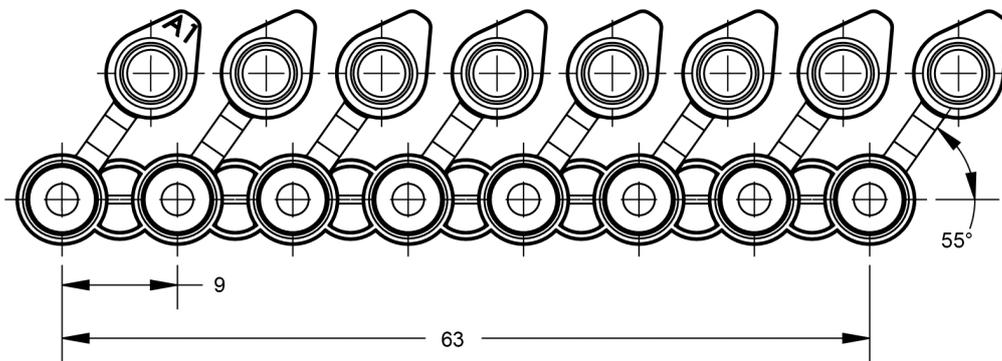

Dimensions in mm

Type	low profile
Volume	0.15 ml / tube
Material	PP
Color	transparent
Cap	attached, flat individual cap
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.




02.51.12.70.01

Batailler-labo.fr



Contact@batailler-labo.fr

Strip of 8 PCR Tubes, 0.2 ml 781320

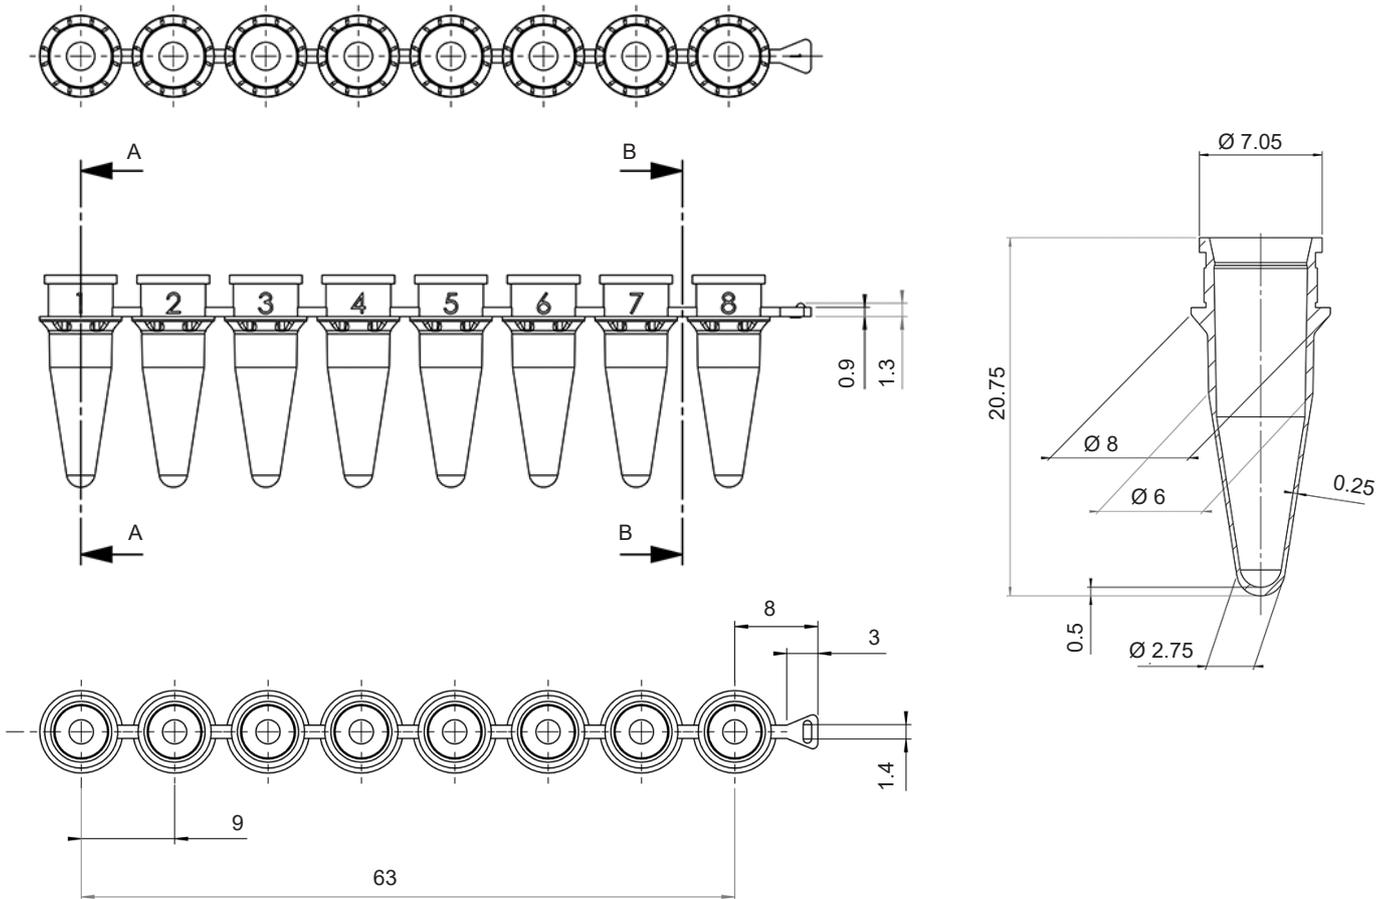

Dimensions in mm



Type	standard
Volume	0.2 ml / tube
Material	PP
Color	transparent
Cap	detached cap strips
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.

Strip of 8 PCR Tubes, 0.2 ml, with cap 781332

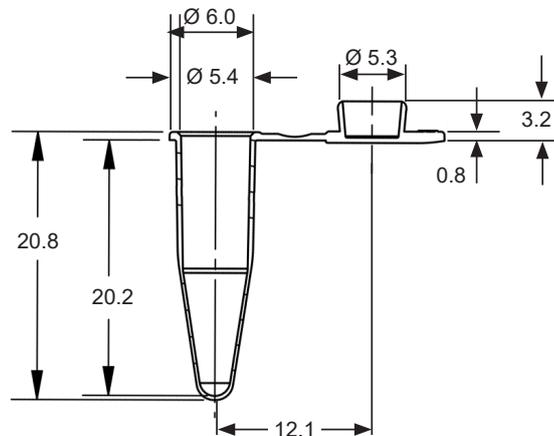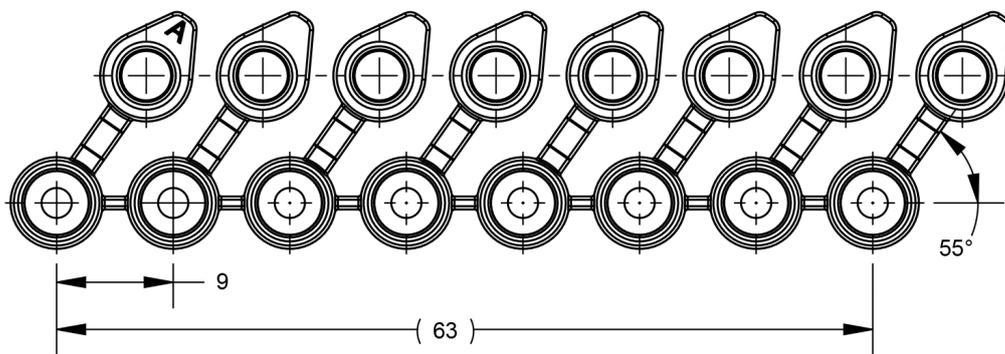

Dimensions in mm



Type	standard
Volume	0.2 ml / tube
Material	PP
Color	transparent
Cap	attached, flat individual cap
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.

Strip of 8 PCR Tubes, 0.15 ml, with cap 781333

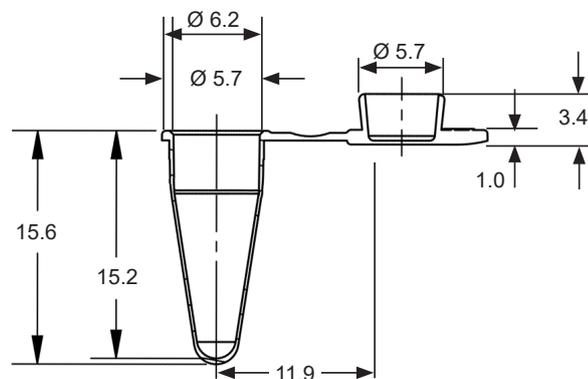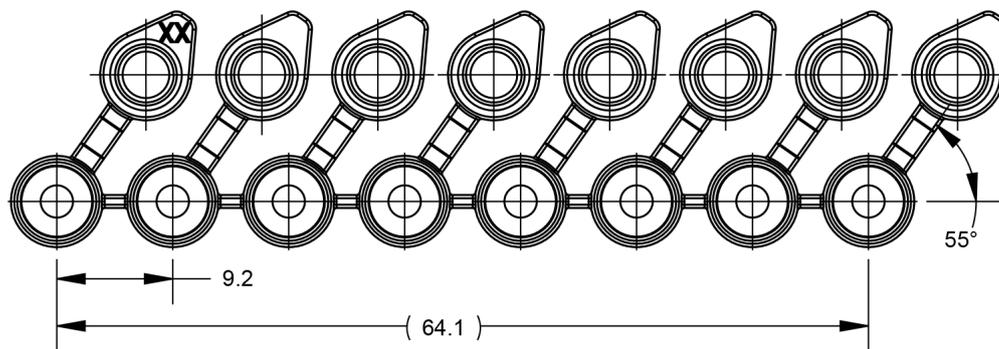

Dimensions in mm

Type	low profile
Volume	0.15 ml / tube
Material	PP
Color	transparent
Cap	attached, flat individual cap
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Free of PCR inhibitors

* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml



Subject to technical modification without notice. Errors excepted.